


Chromatogram and Results

Injection Details

Injection Name:	phenol 50 mg/L	Run Time (min):	21,50
Vial Number:	BA3	Injection Volume:	40,00
Injection Type:	Calibration Standard	Channel:	UV_VIS_1
Calibration Level:	07	Wavelength:	280,0
Instrument Method:	chlorophenol 3D_21,5	Bandwidth:	4
Processing Method:	chlorophenol	Dilution Factor:	1,0000
Injection Date/Time:	18.5.17 14:55	Sample Weight:	1,0000

Chromatogram

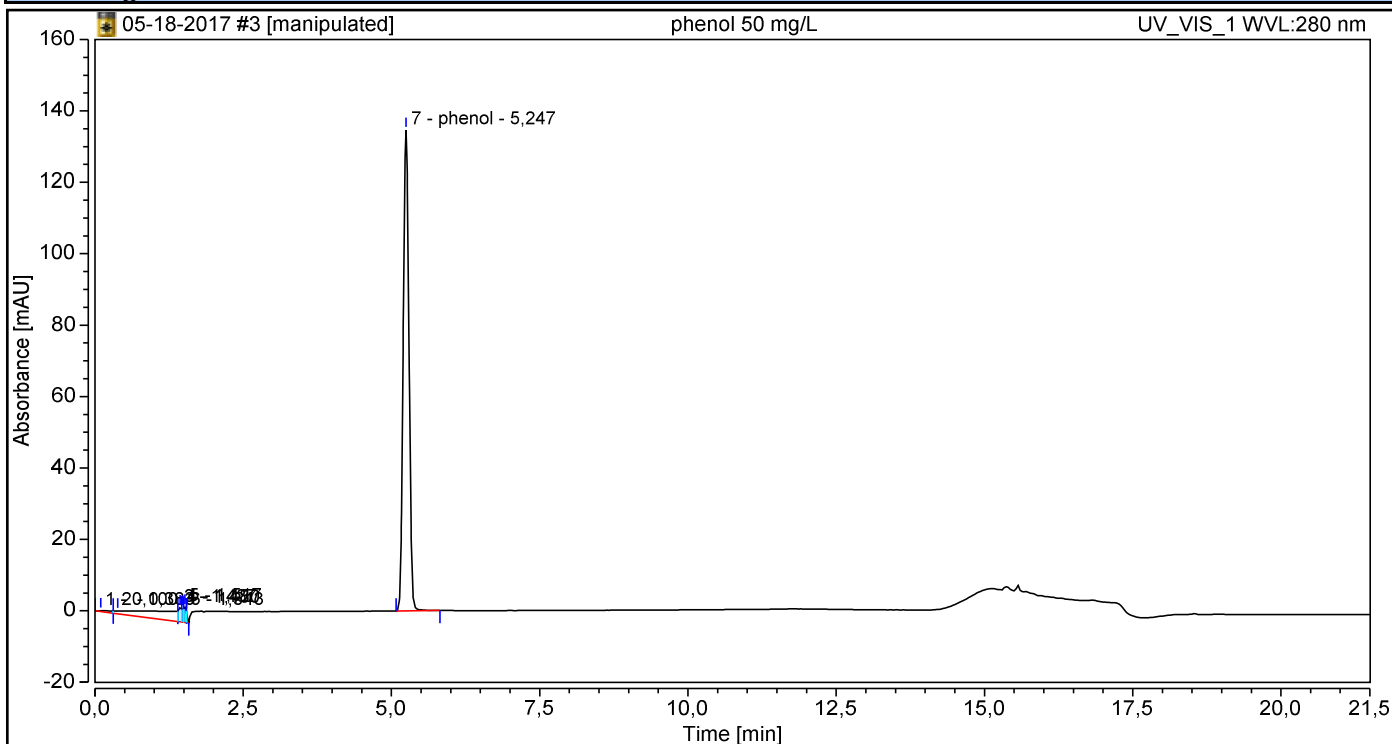

Integration Results

No.	Peak Name	Retention Time min	Area mAU*min	Height mAU	Relative Area %	Relative Height %	Amount mg/L
1		0,100	0,098	0,269	0,55	0,18	n.a.
2		0,383	1,904	0,797	10,78	0,53	n.a.
3		1,437	0,223	3,926	1,26	2,60	n.a.
4		1,480	0,112	3,855	0,63	2,55	n.a.
5		1,517	0,196	4,266	1,11	2,83	n.a.
6		1,543	0,053	3,247	0,30	2,15	n.a.
7	phenol	5,247	15,073	134,622	85,35	89,17	49,8748
n.a.	2-chlorophenol	n.a.	n.a.	n.a.	n.a.	n.a.	n.a.
Total:			17,659	150,981	100,00	100,00	